





4



3.5

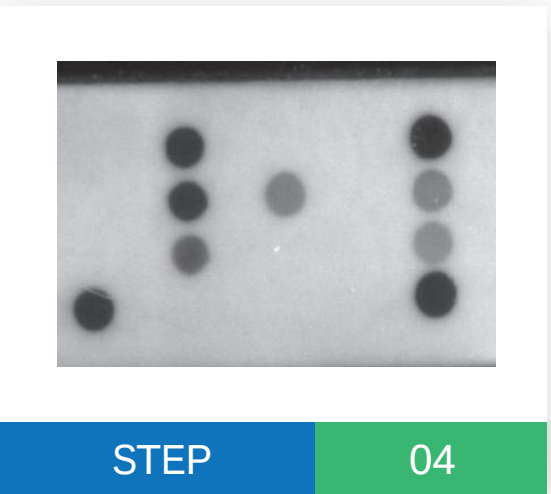

PCR

“ ”

24/28

24 17 HPV 7 , 16 18 HPV
16 58 52 18 33 68 53 66 HPV
28 24 HR-HPV 26 LR-HPV 40 54 61 HPV

17/18

16 18 26 31 33 35 39 45 51 52 53 56 58 59 66 68 73 82

7/10

6 11 40 42 43 44 54 61 81 83

FULLY ENCLOSED

4

4

7cm*8cm

68

合作客户发表文章（部分）	期刊名	发表年份	文章标题
--------------	-----	------	------

Journal of Medical Virology


解放军医学院学报

From

SINGLE-SAMPLE FULL QUALITY CONTROL

GenPlex®

PCR“”4

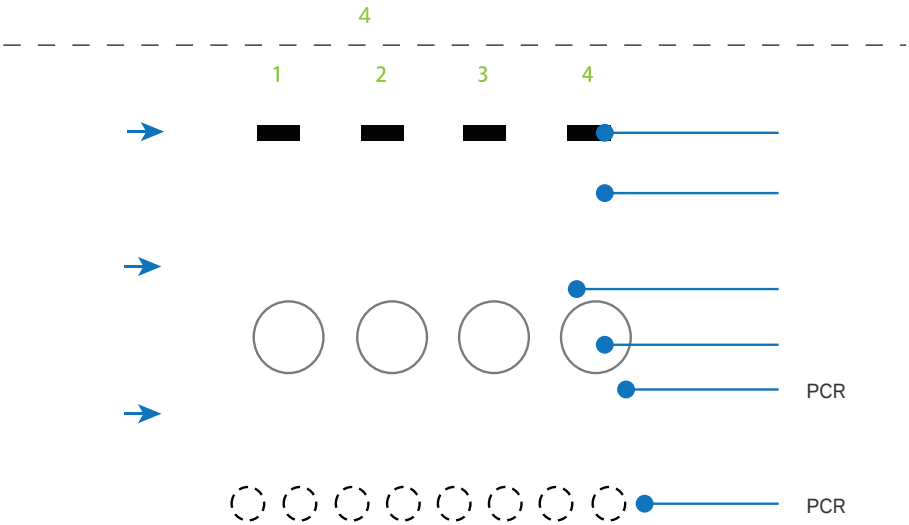

	系统描述	微流控全自动核酸检测系统
	检测通量	24 人份；12 人份；8 人份
	检测时间	4 小时
	试剂包	
		精度：≥ 99.2%
	升降温速率及精确度	平均升温速率：从 50℃～90℃, ≥ 1.5℃ /S 平均降温速率：从 90℃～50℃, ≥ 1.5℃ /S 模块控温

2001

(:300318)

“ ”